




KONICA MINOLTA

Traceability System for Non-Contact 3D Digityzer VI-900 / VI-910

January, 2004

Konica Minolta Photo Imaging Europe GmbH
Instrument Systems Division

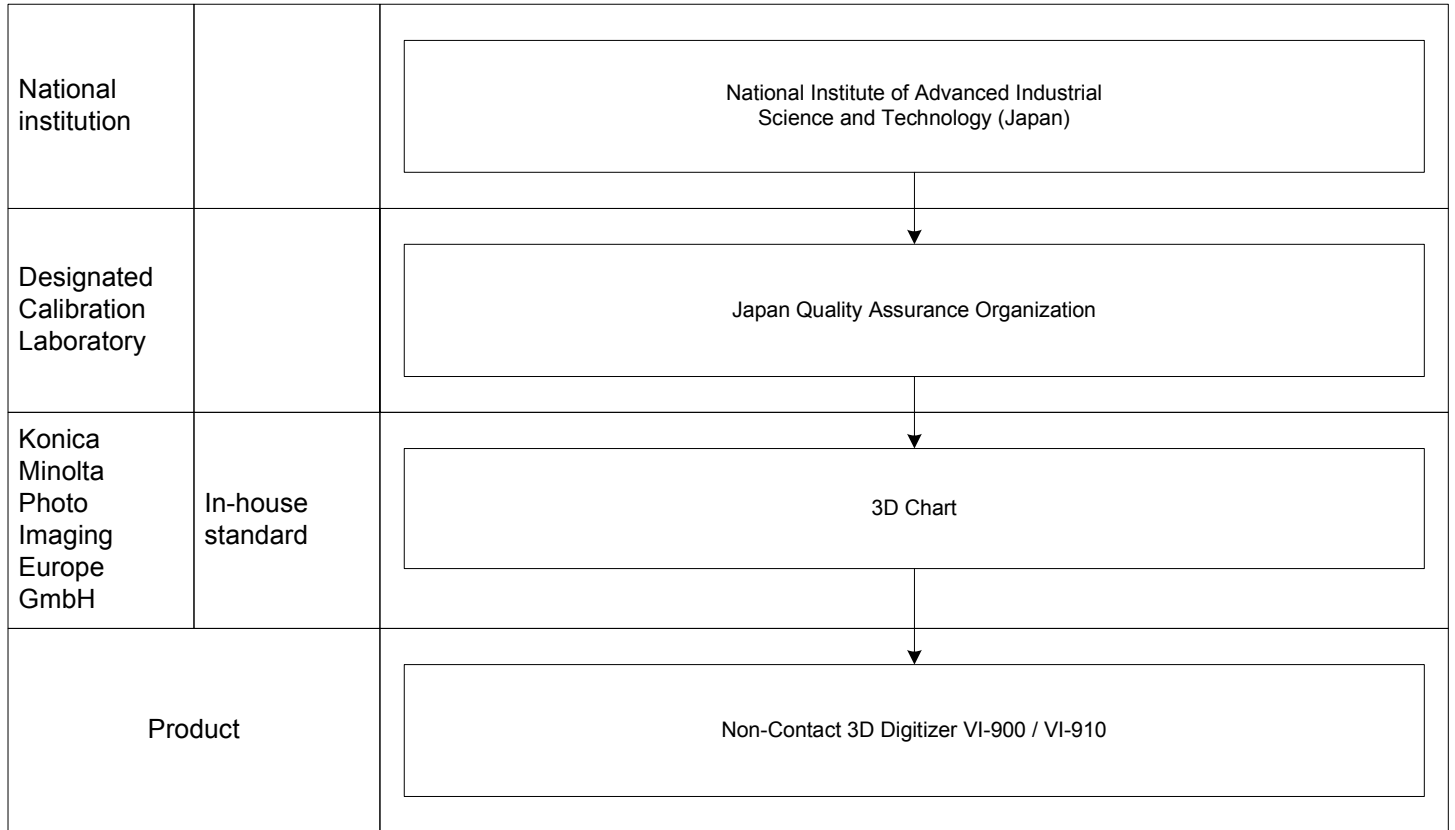

Interval between calibration:
3D Chart : 5 years